

Keep Your Lab Flowing

With RM on Your Agilent 1100 & 1200 HPLC Systems


Routine maintenance (RM) reduces downtime and protects your valuable analytical data. Use this guide to keep your Agilent 1100 and 1200 HPLC Systems operating at their best—replace these crucial components at the recommended intervals and keep extras on hand.

Analytical conditions, mobile phases and additives, sample matrices, and other factors can affect maintenance frequency.

LEARN MORE

For helpful maintenance videos and tips, plus a full list of replacement parts, visit www.restek.com

RESTEK
Pure Chromatography

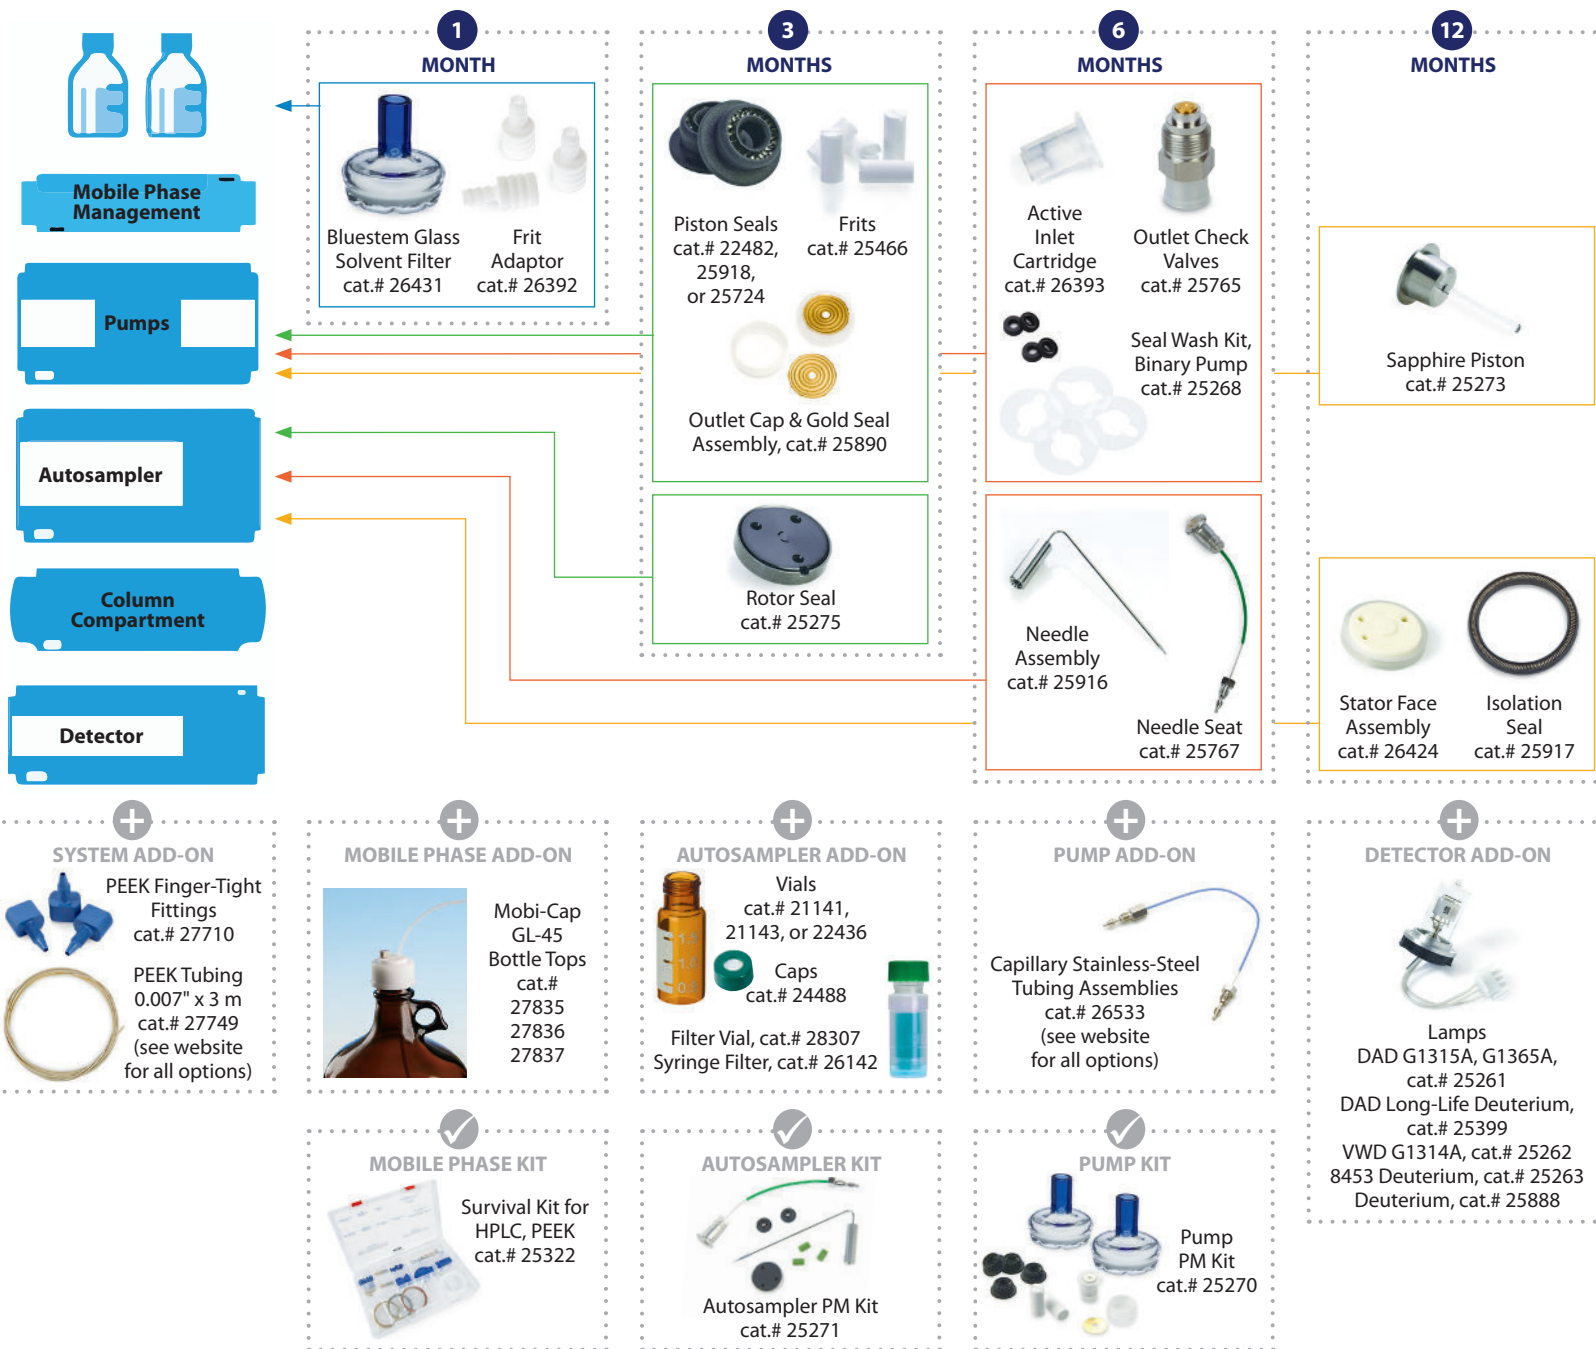

Questions about this or any other Restek product? Contact us or your local Restek representative (www.restek.com/contact-us).

Restek patents and trademarks are the property of Restek Corporation. (See www.restek.com/Patents-Trademarks for full list.) Other trademarks in Restek literature or on its website are the property of their respective owners. Restek registered trademarks are registered in the U.S. and may also be registered in other countries.

© 2023 Restek Corporation. All rights reserved. Printed in the U.S.A.

GN0T3158B-UNV