


Keep Your Lab Flowing

with RM on Your Waters Alliance HPLC Systems

Routine maintenance (RM) reduces downtime and protects your valuable analytical data. Use this guide to keep your Waters Alliance HPLC Systems operating at their best—replace these crucial components at the recommended intervals and keep extras on hand.

Factors such as analytical conditions, mobile phases and additives, and sample matrices can affect maintenance frequency.

For helpful maintenance videos and tips, plus a full list of replacement parts, visit www.restek.com

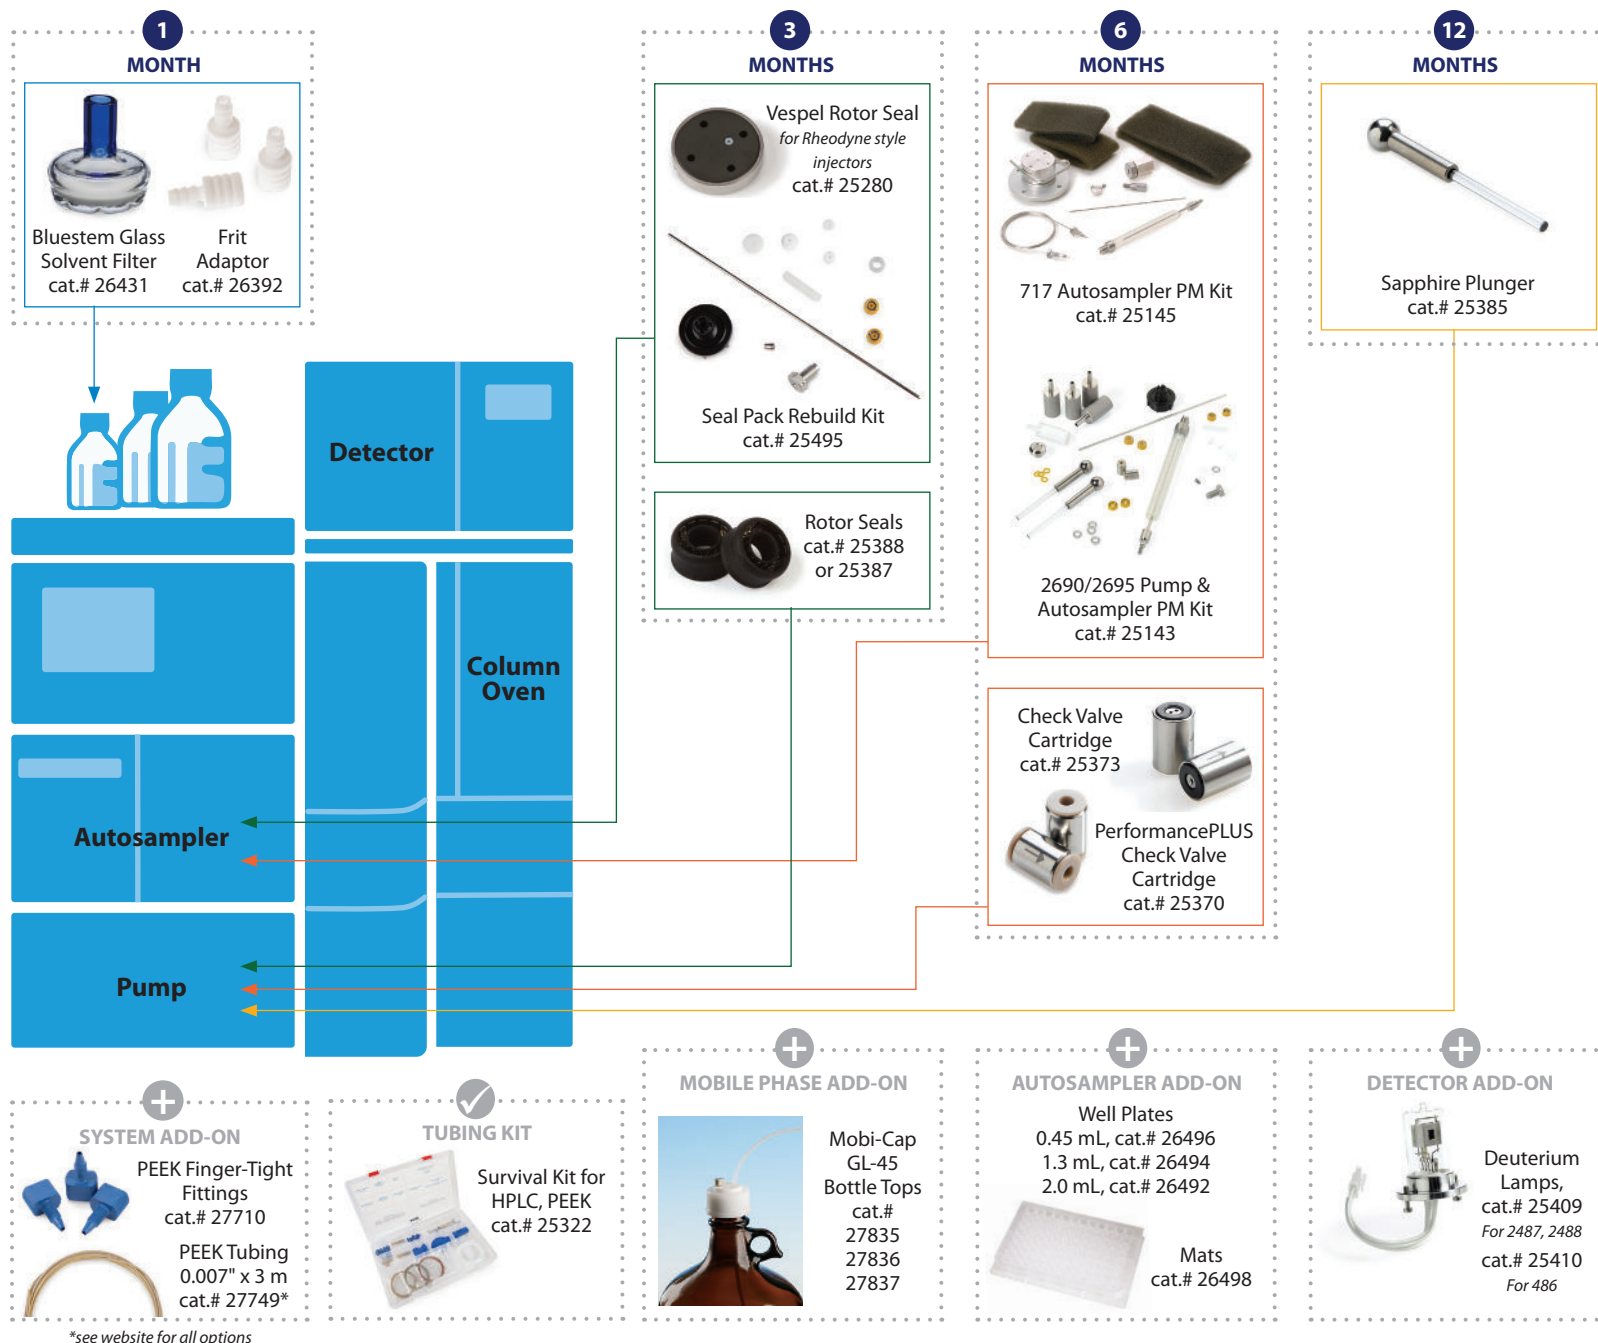

*see website for all options

RESTEK
Pure Chromatography

Questions about this or any other Restek product? Contact us or your local Restek representative (www.restek.com/contact-us).

Restek patents and trademarks are the property of Restek Corporation. (See www.restek.com/Patents-Trademarks for full list.) Other trademarks in Restek literature or on its website are the property of their respective owners. Restek registered trademarks are registered in the U.S. and may also be registered in other countries.

© 2020 Restek Corporation. All rights reserved. Printed in the U.S.A.

GN0T3162-UNV